



*Fixturing systems*

## *Clamping system for computed tomography*

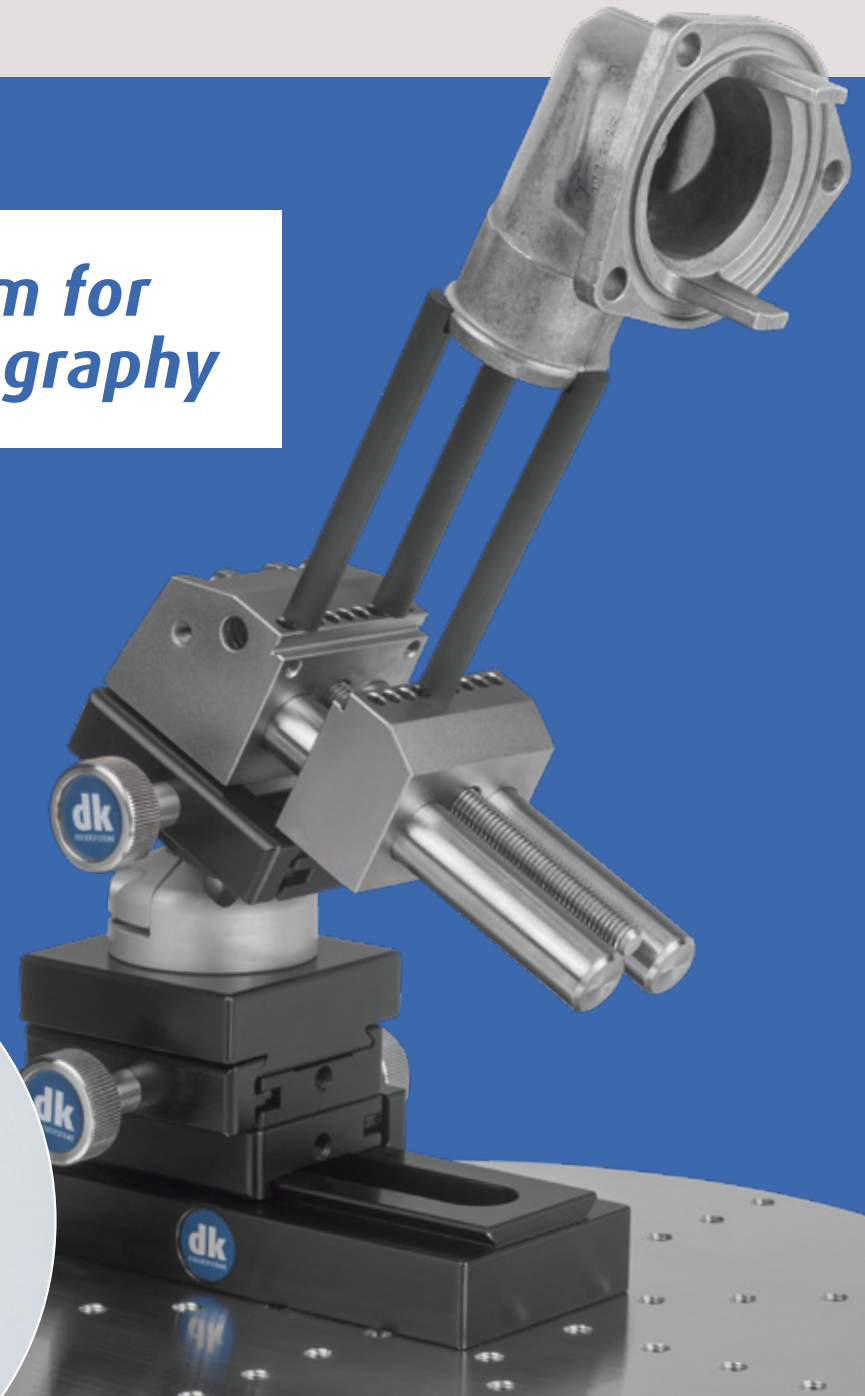

**CT Scan**   
Separation of object  
and fixating system  
through X-ray trans-  
parent connections

# CT scan of components: Quick and simple fixating with X-ray transparent modules from dk

The standard program SWA39 with more than 200 products is the basis for the CT fixating system from dk. In industrial computed tomography, these modules also form the most advanced modular system for clamping devices for the secure holding of all types of parts.

We realise the X-ray transparent connection to the test specimen with workpiece holders that have geometry and materials that create the prerequisite for a CT scan, and which simply and clearly separate the object to be examined from the fixating system.

## Advantages of the dk system

### CT compatible workpiece holder

Modules developed especially, in terms of geometry and materials for industrial computed tomography: completely or, especially in the transition from workpiece to holder, the fixation elements have a significantly lower attenuation coefficient than the test specimen.

The part to be examined is thus clearly distinguishable in the scan. In addition, the geometrically precisely defined clamping elements form the basis for their later exclusion from the overall result if this should become necessary for special parts and processes.

### Professional module system

Precisely coordinated modules are connected via standardised interfaces. Instead of an unstable, short-life and non-adjustable combination of force and form clamping knocked together from soft foams, the dk system enables the professional construction of precise, safe and reusable fixtures.

### Quick, easy and secure construction

The logical separation into adjustment elements, clamping function units and workpiece holders make the system easy to understand and practical for everyone. Each employee can effortlessly assemble a stable clamping fixture in a short time, securely clamp the test piece, align it into position and inclination and readjust it if necessary.

### Repeat accuracy

When several workpieces are to be scanned in series, the clamping position remains identical. This can only ease the testing task.

### Reproducible setups

Fixtures can be completely dismantled and the elements used for other devices. Once constructed, a clamping configuration can be reproduced at any time. Many adjustable elements have scales to aid this.


### Long service life


The basic, clamping and holding elements are wear-resistant. They can therefore be repeatedly used over many years and so, save costs and resources.



### FAST REASSEMBLY LIFELONG

The basic principle of all dk fixating systems. The compatibility of the dk programs makes the utility value perfect.

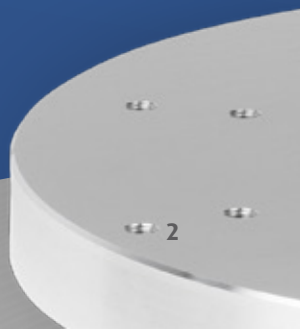

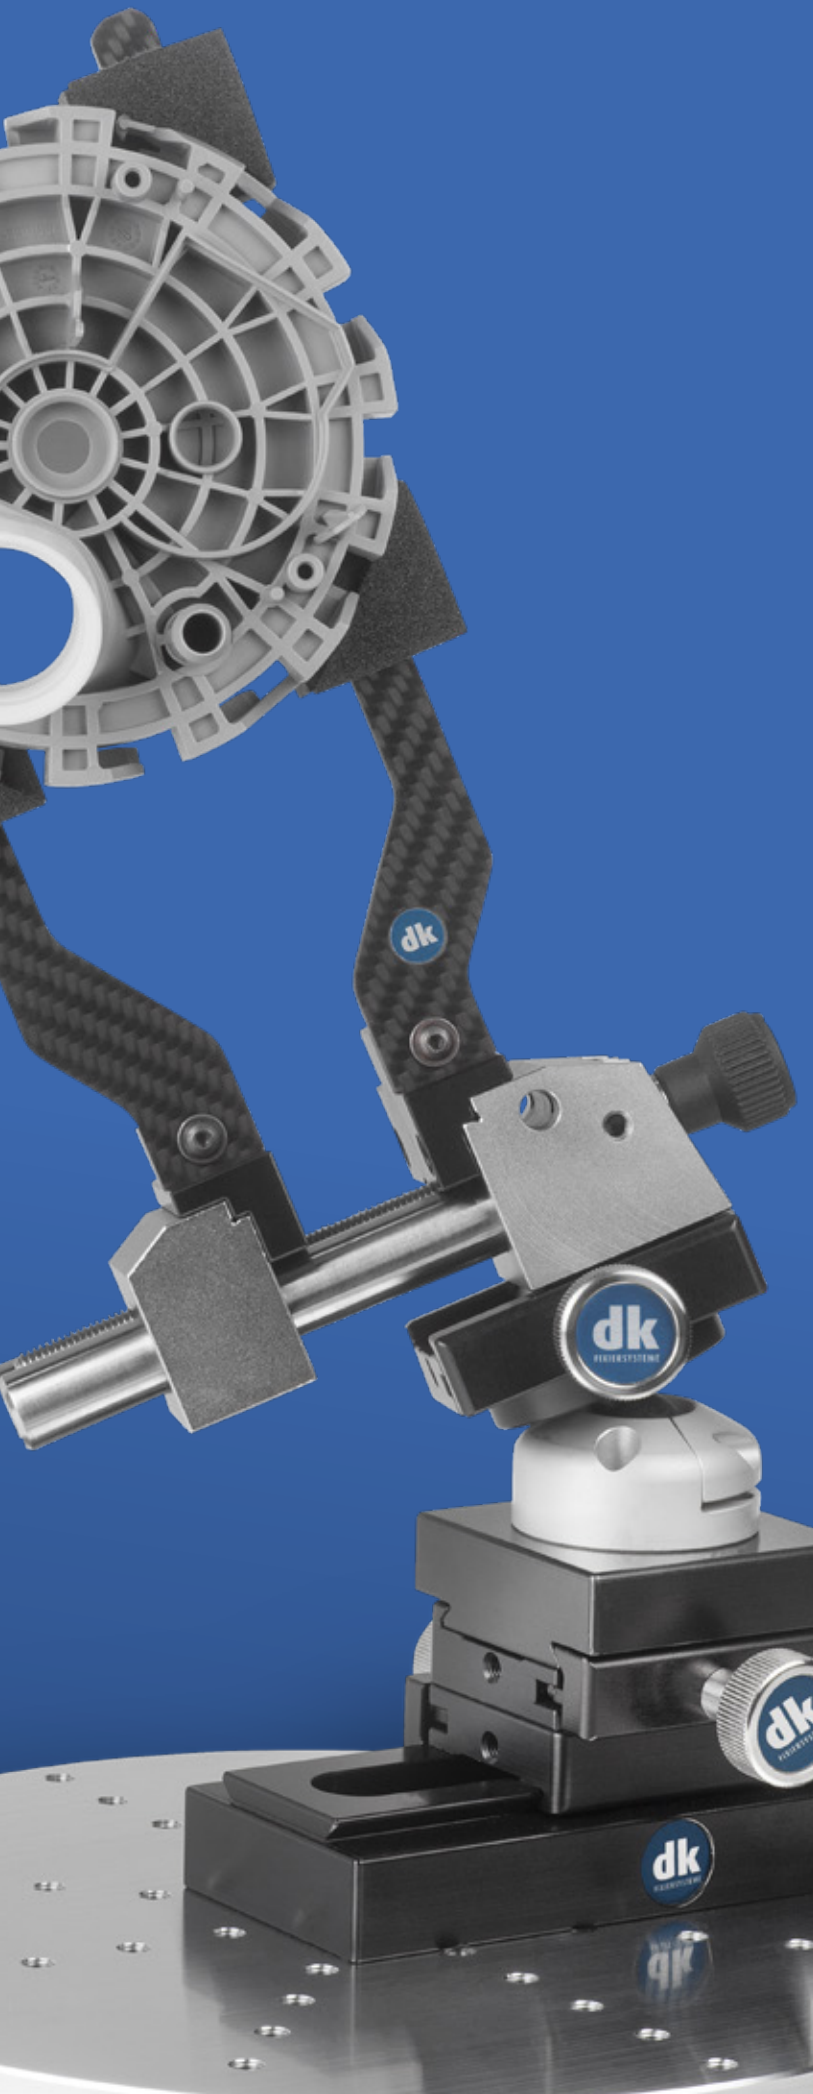

# Contents

## XRAY1

### Predominantly for metal parts

<i>Function principle/Combinations</i>	Page 04
<i>Basic elements Rail system</i>	Page 05
<i>Basic element 3D joints</i>	Page 06
<i>Clamping function elements with SWA39</i>	Page 07
<i>Clamp intermediate elements XRAY1 as CT suitable workpiece holders</i>	Page 08
<i>Small part holder XRAY4 with SWA39</i>	Page 09

## XRAY1+XRS

### Hybrid system predominantly for plastic parts

<i>Function principle/Combinations</i>	Page 10
<i>Clamp intermediate element XRAY1 with foam holder XRS</i>	Page 11

## XRAY4+XRS

### Hybrid small part clamping system

<i>Function principle/Combinations</i>	Page 12
<i>Small part holder XRAY4 with Foam holder XRS and SWA39</i>	Page 13

## XRAY4+XRS

### 3D stand system with hybrid small parts clamp

<i>Function principle/Combinations</i>	Page 14
<i>Small part holder XRAY4 with foam- holder XRS and 3D stand holder</i>	Page 15

#### Publisher

dk FIXIERSYSTEME GmbH & Co. KG,  
Ferdinand-Lassalle-Strasse 35, 72770 Reutlingen, Germany  
info@dk-fixiersysteme.de, www.dk-fixiersysteme.de

#### Status

April 2019

#### Information

With the release of this catalogue, all previous publications become invalid. Dimensions and other data correspond to the current level of technology. We reserve the right to make technical changes. We accept no liability for any printing errors. Any reprinting or reproduction – in whole or in part – is permitted only with our prior consent.

**XRAY1**

# Fixating system with holders for metallic workpieces

## Functioning principle/possible combinations

Metal workpiece or test object


Clamp intermediate element XRAY1 with an attenuation coefficient significantly lower than metal and so clearly distinguishable from the workpiece in the scan

Clamping function element at a clear distance from the workpiece so that no overlapping or interference occurs

3D adjustment unit for infinitely variable and readjustable spatial positioning of the workpiece

Positioning unit, freely positionable, rotatable and movable via slot

Quick change slide adapter, infinitely linear adjustable

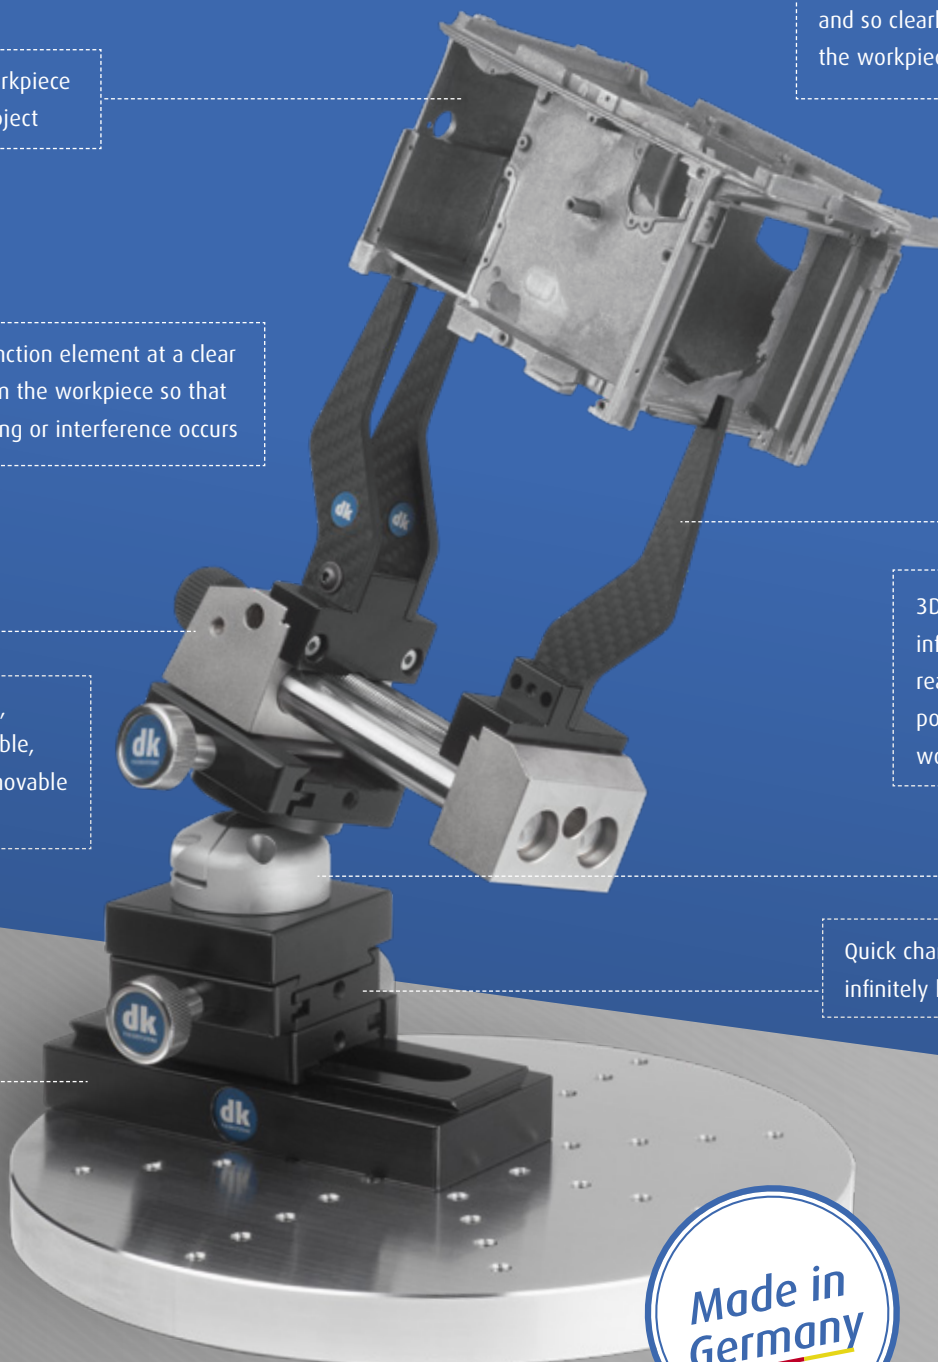

## Rail system for medium and large computed tomography machines

### SWA39 basic rail with slot and SWA39 profile

For locating and basic positioning of the SWA39 quick-change module.

Order No.	BxTxH (mm)
440005	140 x 60 x 20
440000	250 x 60 x 20



### SWA39 Quick change slide adapter

Mounting of SWA39 constructions and their movement on the base rail.

Order No.	BxT (mm)
440010	60 x 110 x 25



### SWA39 quick-action clamp with pivot head

Mounting of SWA39 constructions and their flexible 3D alignment.

Order No.	Description
270550	Rotatable 360° Swivel 30°




### SWA39 Quick-action rotary and pivot unit clamp

Swivels +90° / -55° with worm drive. Infinite rotation through 360° with indexing every 90° (removable) 2° scale, lockable. For spatial alignment of constructions with precisely repeatable setup.

Order No.	Worm drive for...	Length (mm)	Width (mm)	Height (mm)	Fig.
314020	Pivot	85	80	97	1
314030	Rotate and pivot	85	80	116	



### Application example

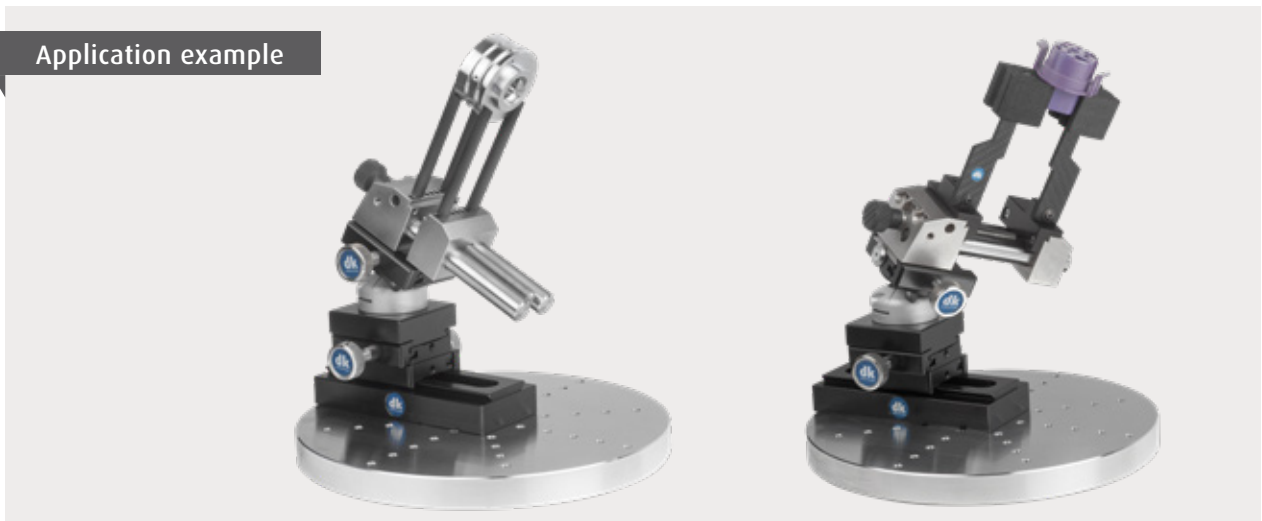

## 3D joint for smaller computed tomography machines

### 3D clamping joint Micro

For mounting an SWA39 adapter. Progressive clamping. Minimum space requirement with maximum freedom and absolute stability. Mounted directly on the baseplate using a satellite mount.



Illustration is with satellite mount and SWA8/M5 adapter

Order No.	Description
440130	Connection: lower M8, upper SWA8

### Horizontal satellite mount for clamping joint

For mounting the clamping joint horizontally on the machine.



Order No.	Description
269700	Fastened to a plate using M6 or M8 screws Fastening joint to satellite mount with M8

### SWA39 Quick-action clamp

For mounting SWA39 constructions. Assembly using SWA/M5 adapter on a clamping joint.



Order No.	Description
273300	Fastening with M5

### SWA8-M5 Adapter

For mounting the quick-change mount on a clamping joint.



Order No.	Description
440135	SWA8 to clamping joint / M5 for quick-change mount

## Application example



## XRAY Clamping function elements with SWA39 interface

### 50 mm precision vice for XRAY element

With special jaw plates for XRAY element. Round elements directly adaptable; flat elements adaptable via system adapter 440035. incl. extension set.

Order No.	Description
440030	Clamping width 35 or 75 mm (with extension)
440035	System adapter for flat clamp intermediate elements XRAY1 (set)



### 65 mm precision three-jaw chuck for XRAY elements

With special jaw plates for XRAY element. Round elements directly adaptable; flat elements adaptable via system adapter 440025.


Order No.	Description
440020	Effective clamping width dependant on clamp intermediate elements
440025	System adapter for flat clamp intermediate element XRAY1 (set)



### 100 mm precision three-jaw chuck for XRAY elements

With special jaw plates for XRAY element. Round elements directly adaptable; flat elements adaptable via system adapter 440025.

Order No.	Description
440015	Effective clamping width dependant on clamp intermediate elements
440025	System adapter for flat clamp intermediate element XRAY1 (set)

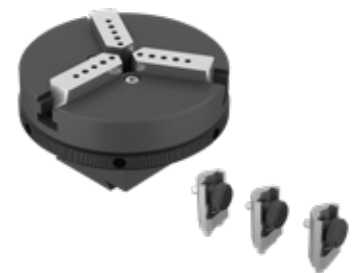

### NADELFIX 2.5 XRAY

Needle cushion with lockable XRAY1 pins for fixed-variable self-moulding of free-form parts. complete with XRAY1 column and XRAY4 needle holder.

Order No.	Description
440125	Active surface ca. 38x38 mm. XRAY1 plunger with low attenuation coefficient



### Application example




# Clamp intermediate element

## XRAY1 clamp intermediate element as CT suitable workpiece holder

### Round clamp intermediate element XRAY1, 80 mm

Direct fastening on XRAY precision vice or XRAY chuck.


Order No.	Description	Fig.
440040	Set with 4 straight offset pin columns	1
440045	Set with 2 inclined offset pin columns as a prism pair.	2

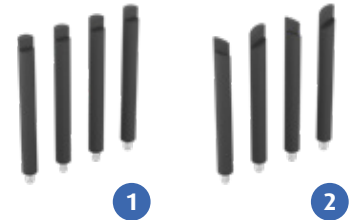

### Flat clamp intermediate element XRAY1 SP straight offset, 100 mm

Fastened using system adapter on XRAY vice or XRAY chuck.

Order No.	Description	Fig.
440055	Straight jaws with step, pointed seating ledges	1
440060	Straight jaws with step, pointed seating ledges clamping width extension 20 mm per jaw	2



### Flat clamp intermediate element XRAY1 with 3 prisms, 100 mm

Fastened using system adapter on vice or chuck.

Order No.	Description
440050	Prism jaws with 3 prism sizes



### Application example





## Piko clamp XRAY4 with SWA39 interface

### Piko clamp top face prism XRAY4 with SWA39

For clamping tiny metallic parts. With integrated vertical prism. For smooth parts or small diameters.

Order No.	Description
440085	Spring-loaded small parts clamp, flat incl. prism



### Piko clamp internal clamping XRAY4 with SWA39

For holding metallic workpieces on the ID.

Order No.	Description
440095	Spring-loaded small parts clamp with two offset diameters 5 and 11 mm



### Application example



# Hybrid holder for scanning engineering plastic

## Functioning principle/possible combinations

XRS stable moulded foam clamp intermediate element mounted on the XRAY1 but with an attenuation coefficient similar to polystyrene foam. The workpiece therefore only comes into direct contact with a non-detectable material and consequently can be clearly distinguished in the scan

Clamping function element at a clear distance from the workpiece so that no overlapping or interference occurs


Quick change slide adapter, infinitely linear adjustable

Engineering plastic workpiece or test object

Clamp intermediate element XRAY1 with an attenuation coefficient significantly lower than metal, which causes no interferences

3D adjustment unit for infinitely variable and re-adjustable spatial positioning of the workpiece

Positioning unit, freely positionable, rotatable and movable via slot

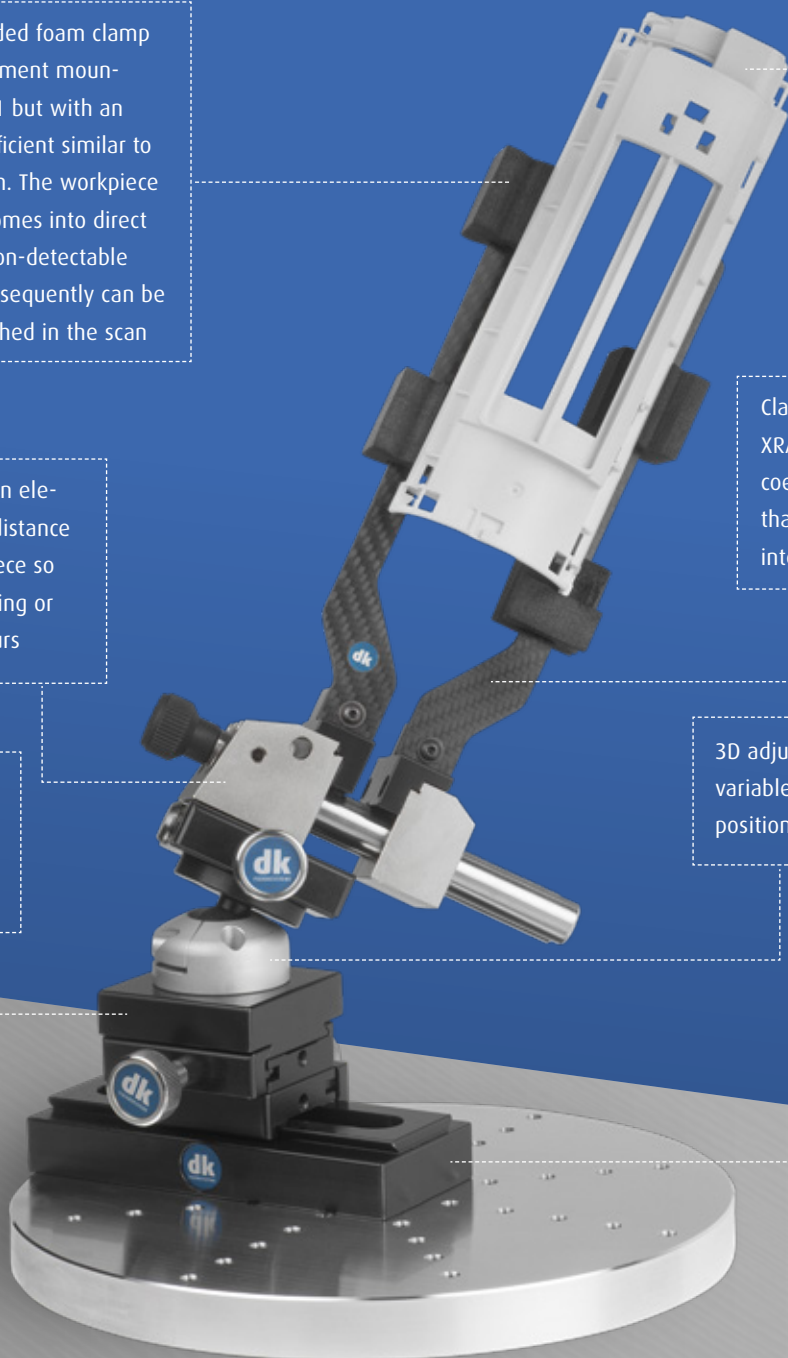


## Clamp intermediate element XRAY1 and foam holder XRS

### Flat clamp intermediate element straight XRAY1 for XRS, 100 mm

Fastened using system adapter on XRAY vice or XRAY chuck


Order No.	Description	Fig.
440065	Form foam element XRS, push-on and infinitely adjustable	1
440070	Form foam element XRS, push-on and infinitely adjustable, clamping width extension 20 mm per jaw	2



### Flat clamp intermediate element straight XRAY1 for XRS, 200 mm

Fastened using system adapter on XRAY vice or XRAY chuck.


Order No.	Description	Fig.
440075	Form foam element XRS, push-on and infinitely adjustable, clamping width extension 20 mm per jaw	1
440080	Form foam element XRS, push-on and infinitely adjustable, clamping width extension 40 mm per jaw	2

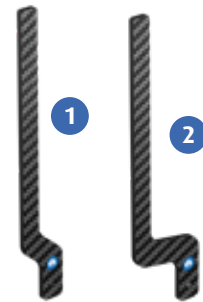


### XRS prism 303030 CT form foam with high strength by low attenuation coefficient

For a simple push-fit on the flat clamp intermediate element for XRS, self-locking, rotatable through 180° and inclinable: The workpiece has no direct contact to a material with similar attenuation coefficient and consequently is clearly distinguishable.

Order No.	Description	Fig.
440110	XRS form foam cube 30x30x30 mm with a large prism	1
440115	XRS form foam cube 30x30x30 mm with 4 small prisms	2

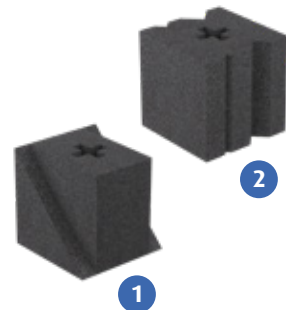

### Application example

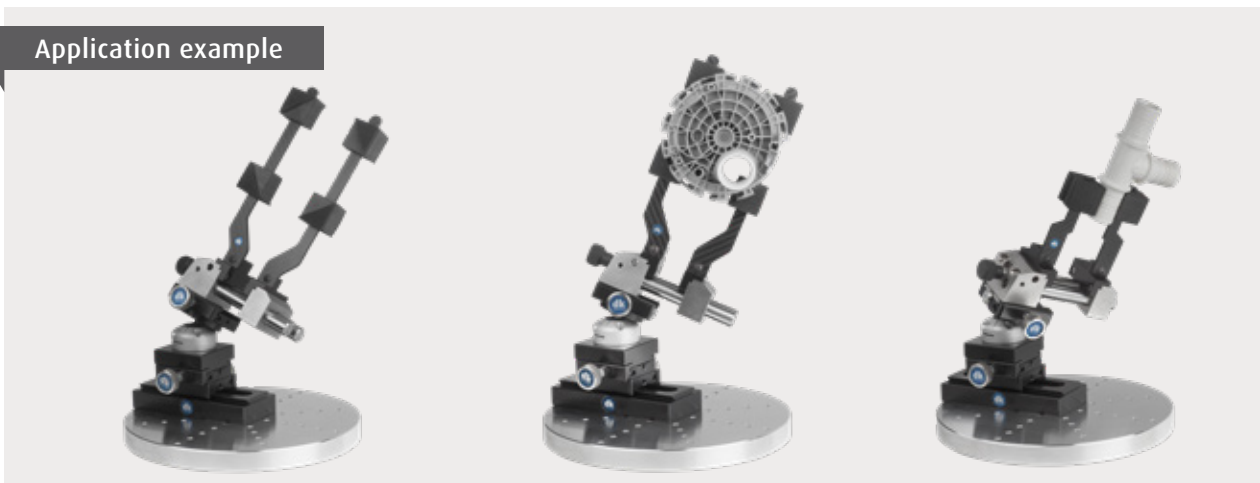


# Hybrid small parts clamp for scanning engineering plastic

Functioning principle/possible combinations



Snapshot from the test series: XRS clamp intermediate element as stable moulded foam mounted on the Piko clamp from XRAY4. The largely neutral Piko clamp causes no interference. The special foam XRS has an attenuation coefficient similar to polystyrene...

...the workpiece therefore only comes into direct contact with a non-detectable material and is thereby clearly distinguishable in the scan: the test piece is virtually suspended in the air!

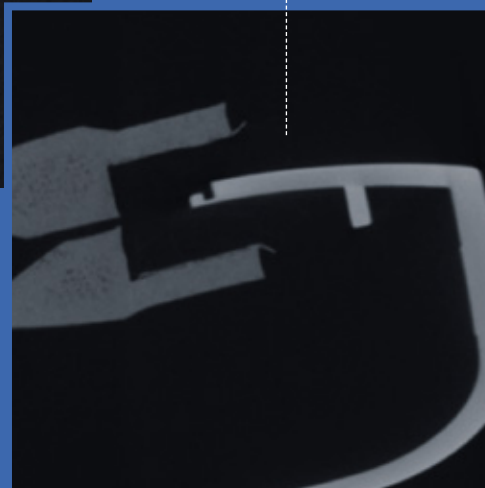

## Piko clamp XRAY4 with XRS foam attachment and SWA39 interface

### Piko clamp XRAY4 for XRS

For mounting 2 CT moulded foam elements with high strength by low attenuation coefficient. For clamping tiny plastic parts.

Order No.	Description
440090	Spring-loaded small parts clamp incl. CT moulded foam attachment, attachment with asymmetrical opening for setting 3 clamping widths, 0 - 2.5 mm, 2.5 - 5 mm and 5 - 7.5 mm. Customer-specific foam inserts can be glued on.




### XRS system foam attachment

To push-fit onto the Piko clamp 440090. High strength by low attenuation coefficient. Adjustable for various workpiece thicknesses from 0 to 7.5 mm by rotating the asymmetrical opening by 180°.

Order No.	Description
440120	1 pair of XRS foam attachments with asymmetrical openings for setting 3 clamping widths, 0 - 2.5 mm, 2.5 - 5 mm and 5 - 7.5 mm.



### Application example

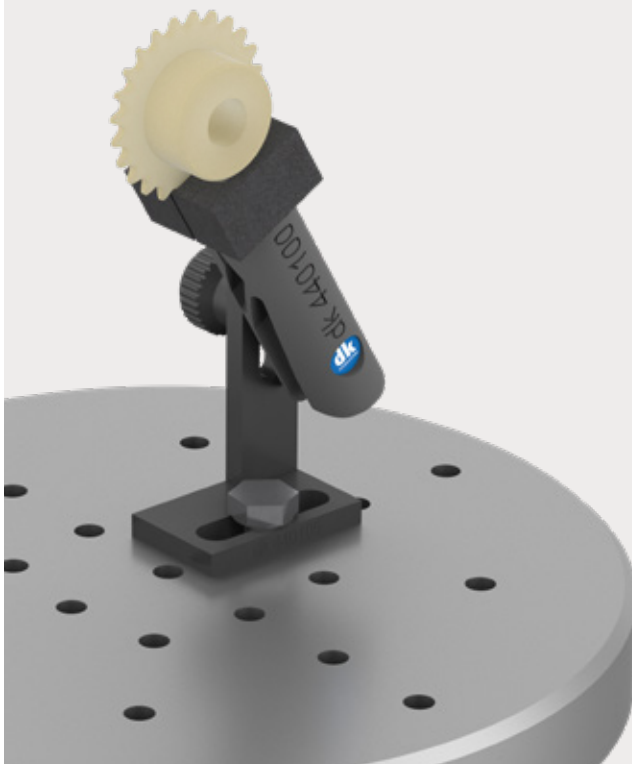

**XRAY4<sup>+XRS</sup>**


# 3D stand system with hybrid small-parts clamp

Functioning principle/possible combinations

Engineering plastic workpiece  
or test object

Piko clamp as hybrid element  
from XRAY4 with XRS foam at-  
tachment. The basic holder makes  
the small parts clamp height-  
adjustable, inclinable, movable  
and rotatable

The holder itself can be rotated  
and moved in order to position  
the test piece in the centre

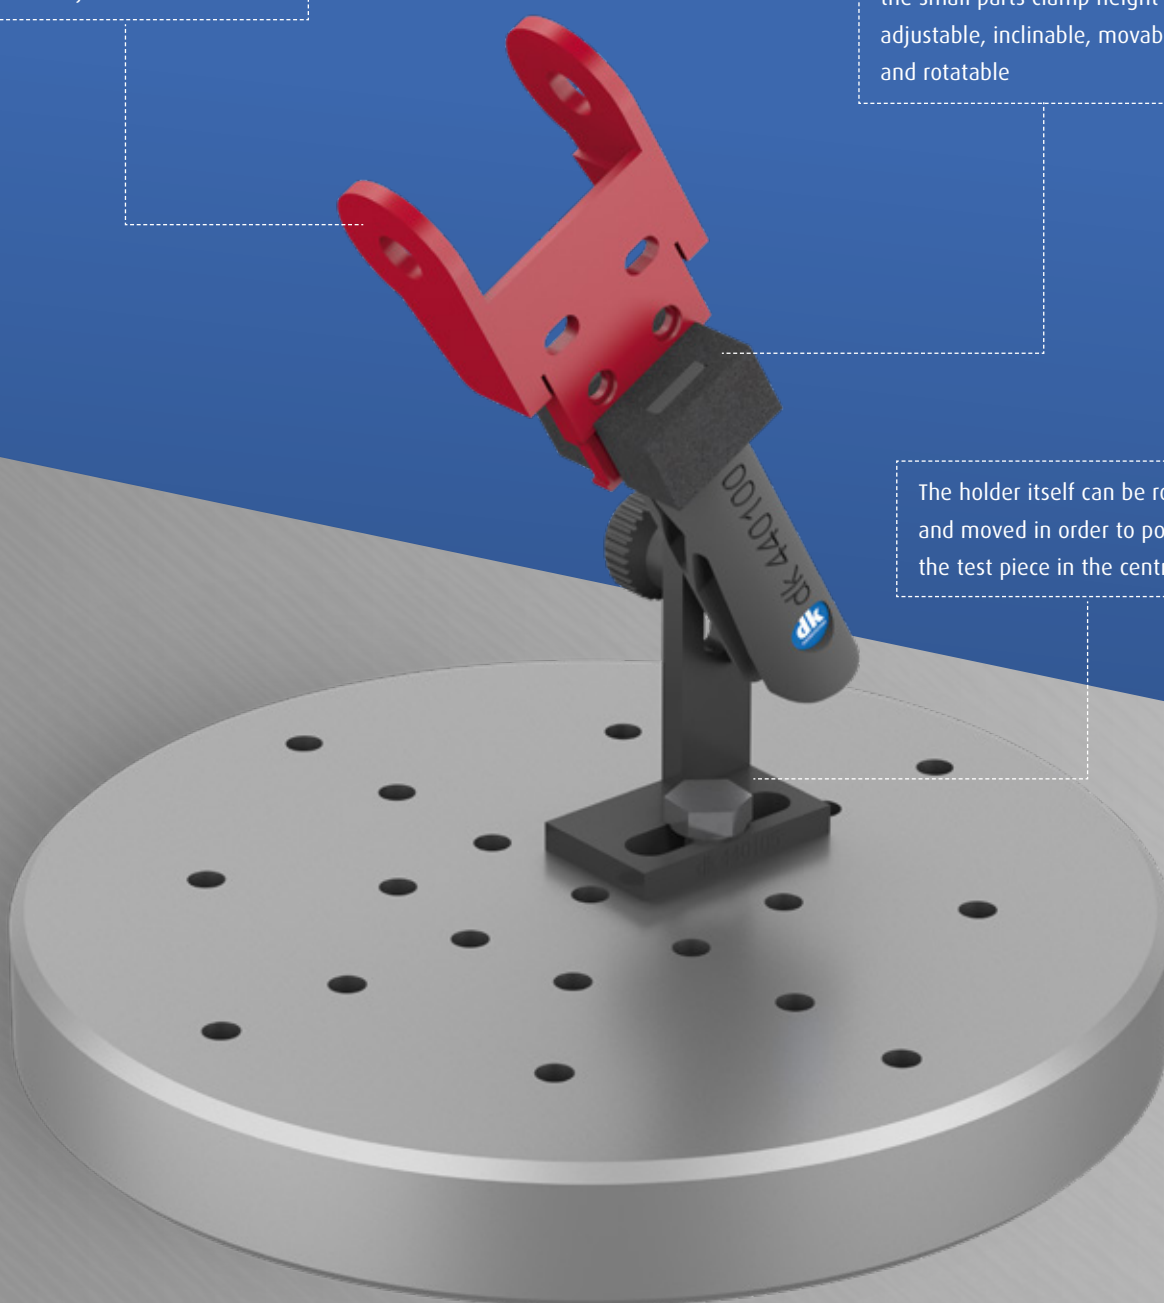

## Piko clamp XRAY4 with XRS foam attachment and 3D stand holder

### 3D stand holder for Piko clamp without SWA39

For height-adjustable and inclinable mounting of the Piko clamps without SWA39. For mounting on a base plate, can be moved and rotated via the slot.

Order No.	Description
440105	3D stand holder with rotation and movement via horizontal slot as well as inclination and height-adjustable mounting for small parts holder via vertical slot.



### Piko clamp XRAY4 for XRS without SWA39 for 3D stand holder

For mounting 2 CT moulded foam elements with high strength by low attenuation coefficient. For clamping tiny parts.


Order No.	Description
440100	Spring-loaded small parts clamp incl. CT moulded foam attachment, attachment with asymmetrical openings for setting 3 clamping widths, 0 - 2.5 mm, 2.5 - 5 mm and 5 - 7.5 mm. Customer-specific foam inserts can be glued on. For mounting on holder 440105, height-adjustable and inclinable.



### XRS system foam attachment

To push-fit onto the Piko clamp 440100. High strength by low attenuation coefficient. 180° rotatable for various workpiece thicknesses from 0 to 7.5 mm.

Order No.	Description
440120	1 pair of XRS foam attachments with asymmetrical openings for setting 3 clamping widths, 0 - 2.5 mm, 2.5 - 5 mm and 5 - 7.5 mm.

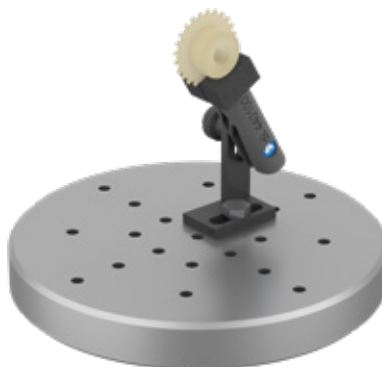



The digital version of our  
catalogue is available here:  
[www.dk-fixiersysteme.de](http://www.dk-fixiersysteme.de)

**dk**  
FIXIERSYSTEME

dk FIXIERSYSTEME GmbH & Co. KG  
Ferdinand-Lassalle-Straße 35  
72770 Reutlingen, Germany

Tel. +49 (0) 7121 90 97 10  
Fax +49 (0) 7121 90 97 120  
[www.dk-fixiersysteme.de](http://www.dk-fixiersysteme.de)  
[info@dk-fixiersysteme.de](mailto:info@dk-fixiersysteme.de)

# The entire world of fixating, clamping and positioning.


## SWA39

Quick-change system for  
tactile and optical measuring




## SPANNFIX PRO

Professional clamping system  
for tactile measuring




## SPANNFIX ECO

Economic clamping system  
for tactile measuring




## QUADERFIX

3D clamping system for  
tactile measuring




## SCHIENENFIX

Clamping system for optical  
and multi-sensorial measuring




## MICROFIX

Clamping solutions for  
micro parts



## SPEZIALFIX

Customer-specific  
clamping fixtures



*modular. simple. better.*